


-15kV TOF: -9116 v
 -3.6kV MCP: -2782 v
 -2.4kV MCP: -1579 v
 Input Cur: 302 ma
 RPA max: 237 v
 Mirror max: 238 v

Mon Sep 25 11:05:49 2006

TIDE Direct Events

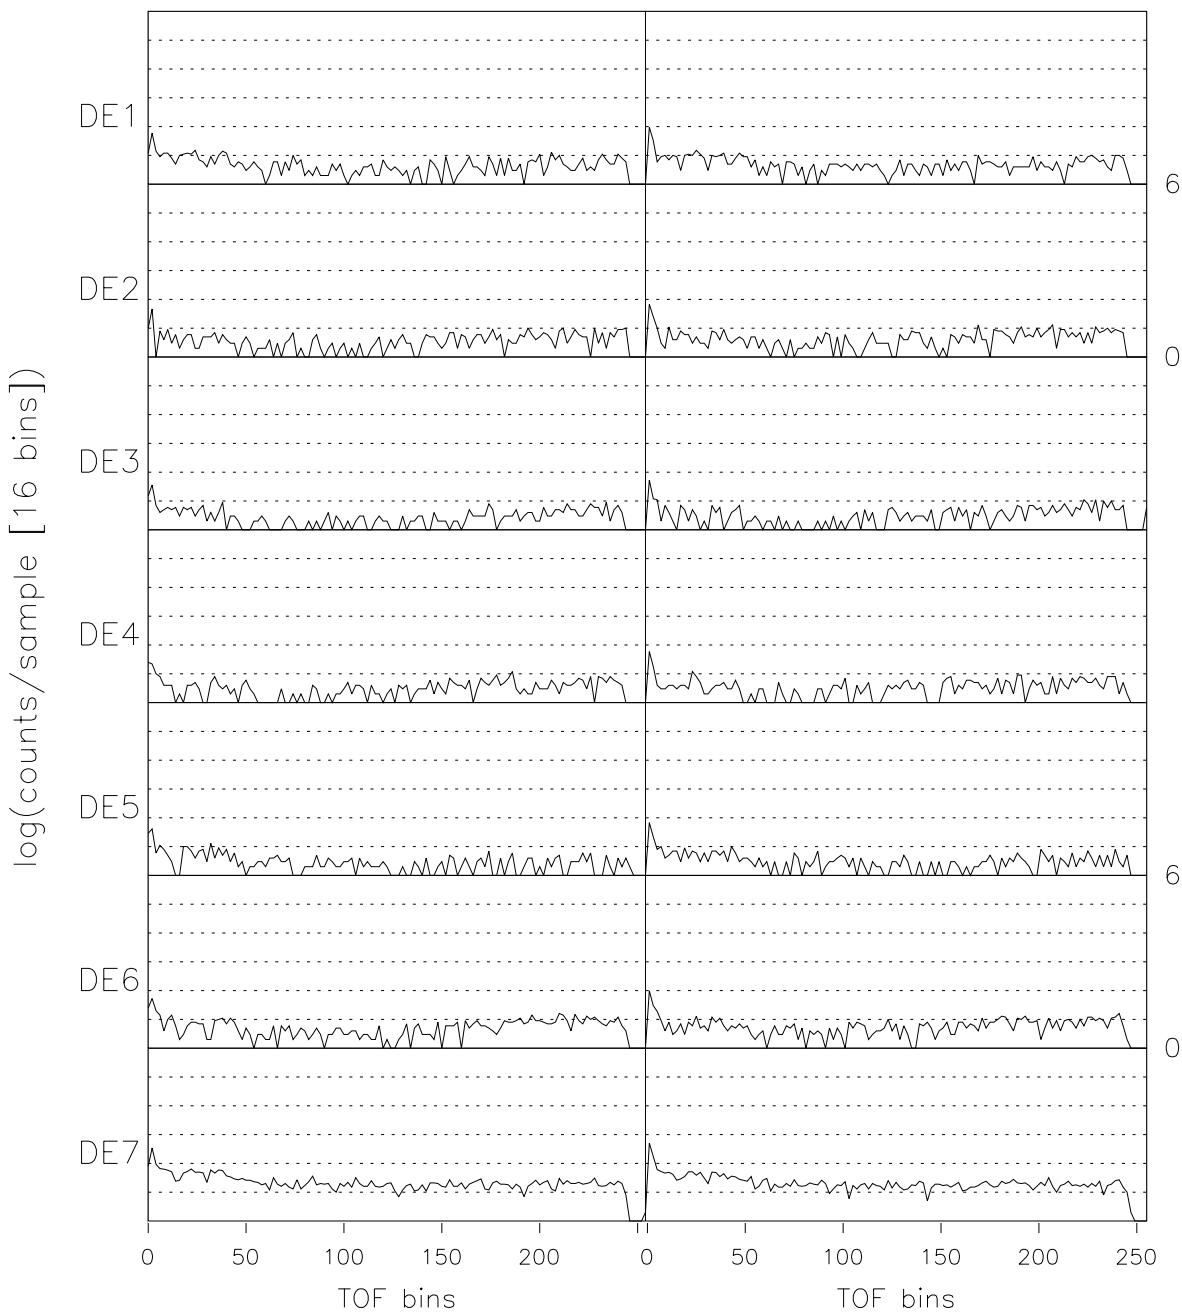

reported: 09-26-96 20:24:47 UT

reported: 09-26-96 20:27:59 UT

file: /export/data/tide/nrt/96092601.dat

-15kV TOF: -9116 v

-3.6kV MCP: -2578 v

-2.4kV MCP: -1579 v

Input Cur: 300 ma

RPA max: 237 v

Mirror max: 238 v